


FIG.1

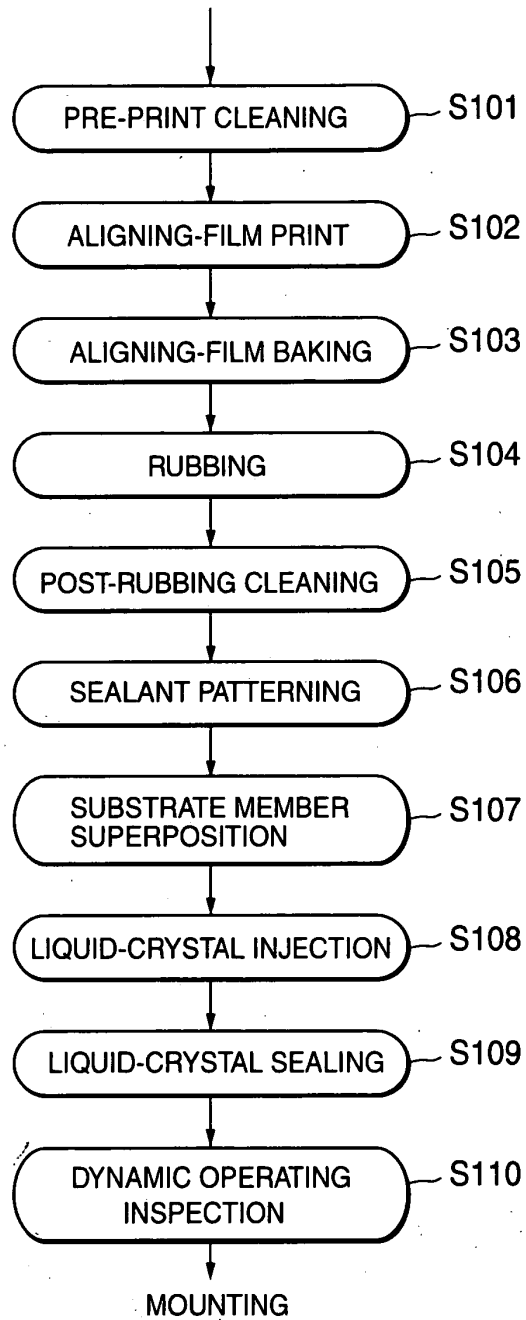

T00221" TEE2200T

FIG.2

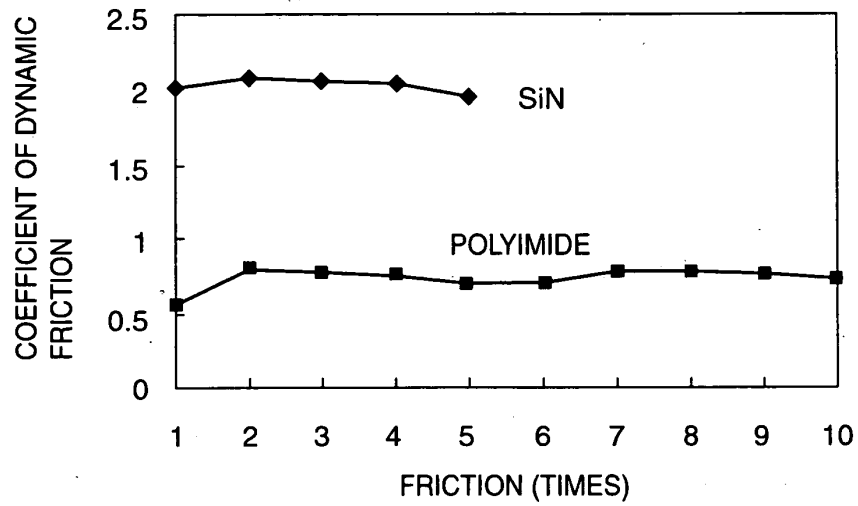


FIG.3

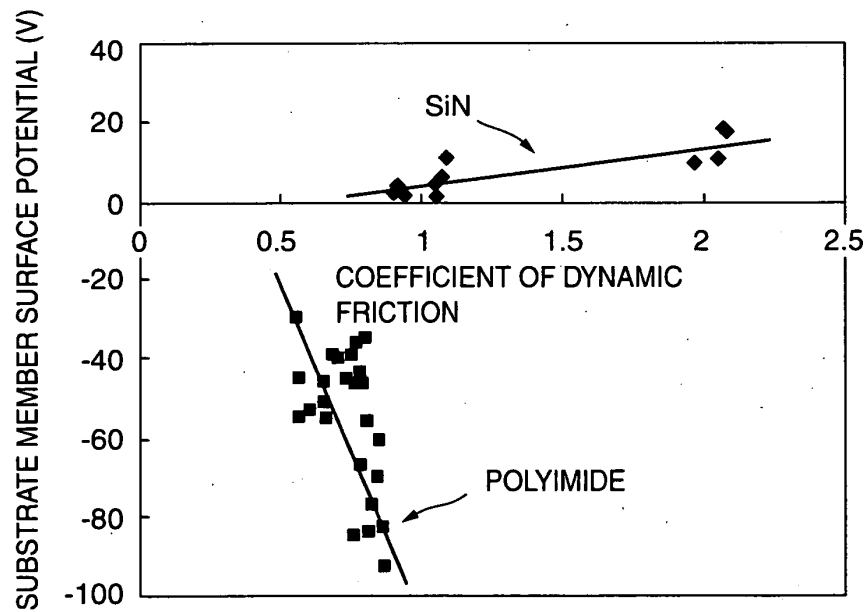


FIG.4

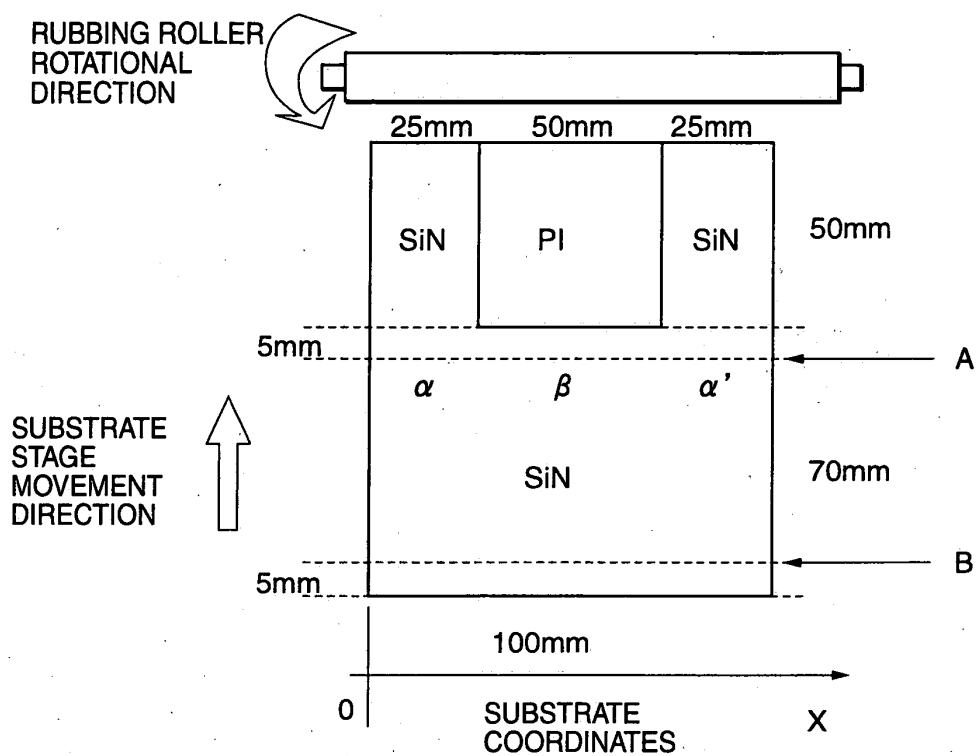


FIG.5


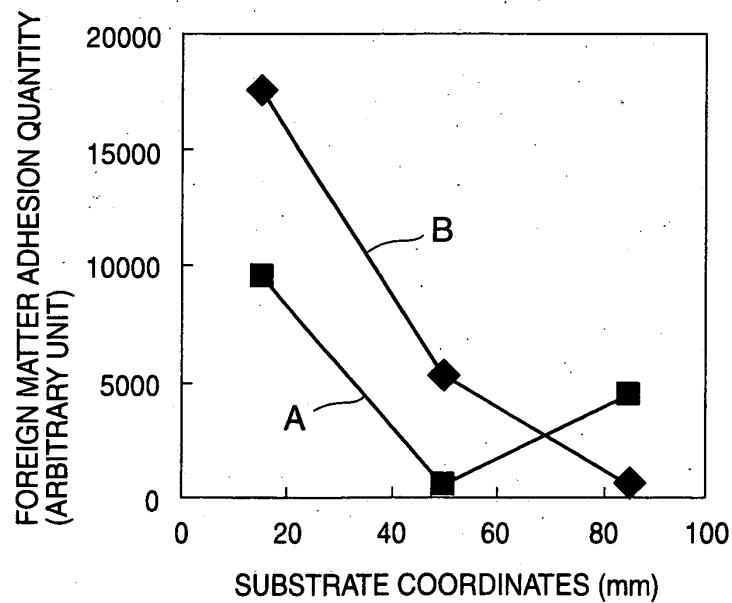


FIG.6

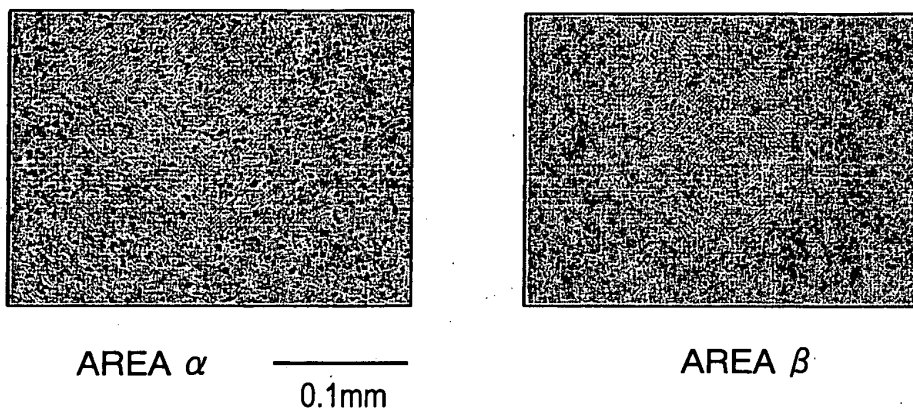

OPTICAL-MICROPHOTOGRAPH IMAGE  
OF FOREIGN MATTER HAVING ADHERED

100221-12201

FIG.7

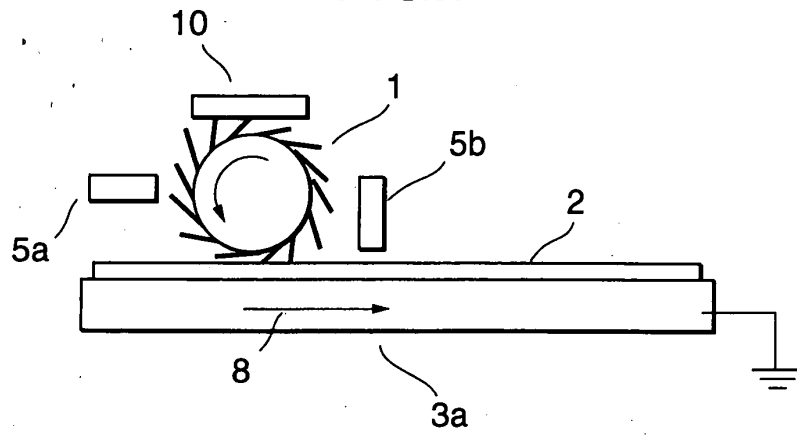


FIG.8

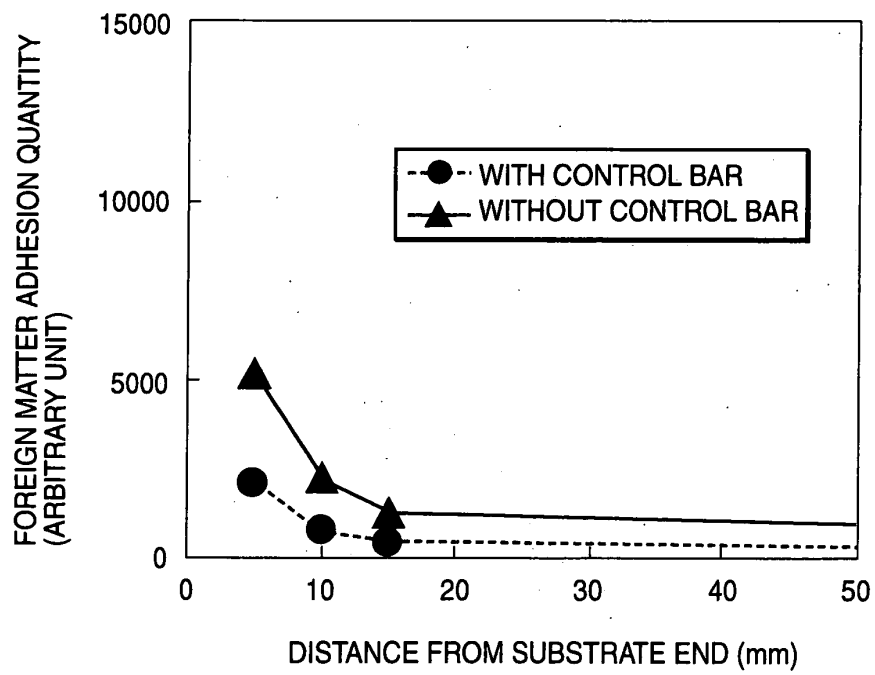


FIG.9

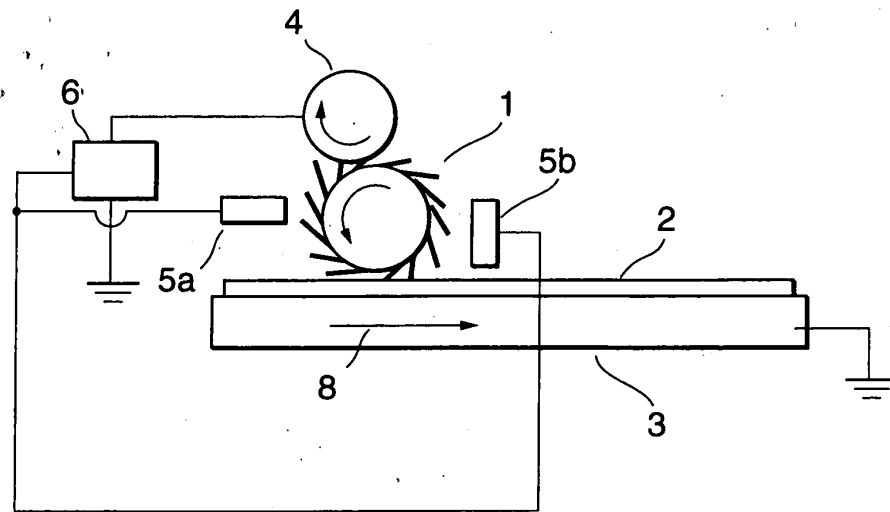


FIG.10

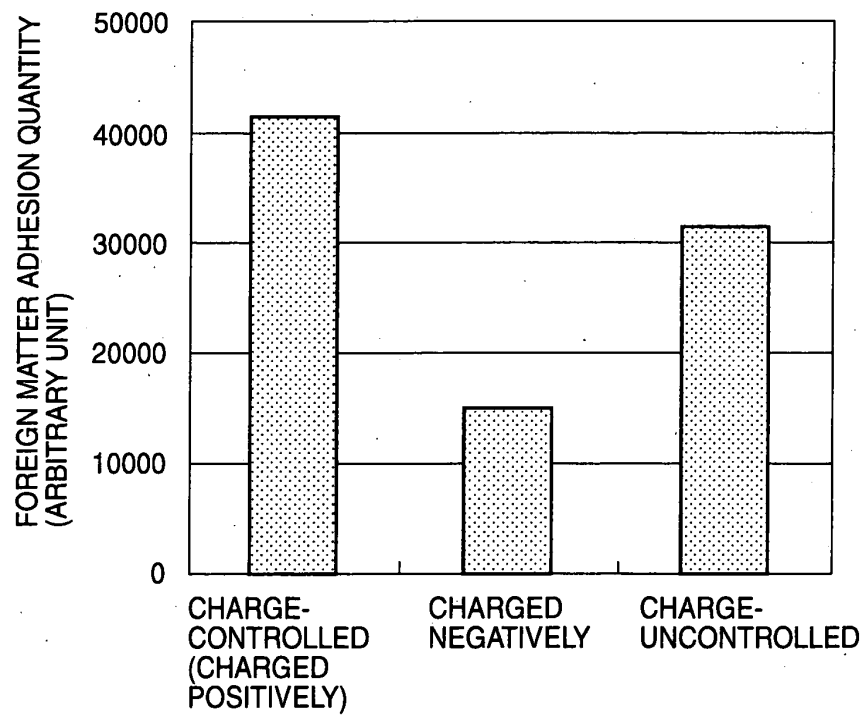


FIG.11

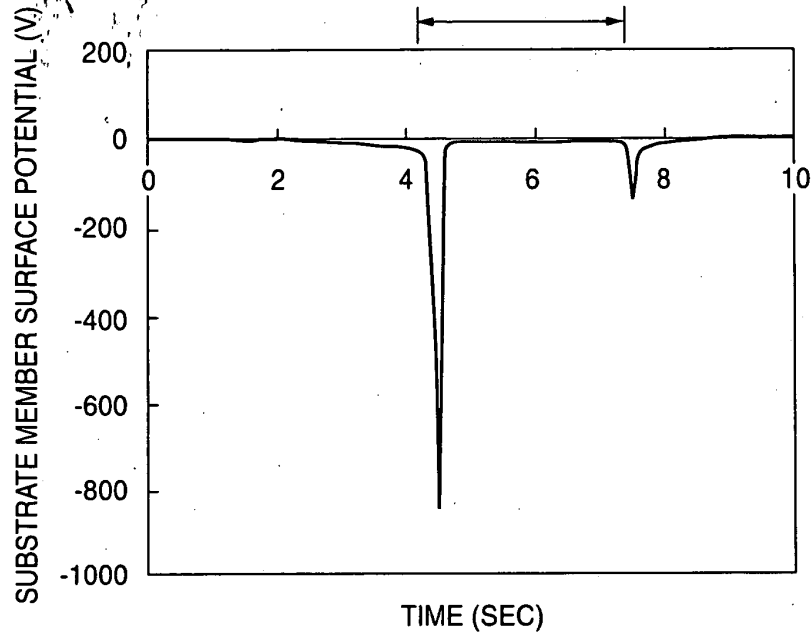
MEASUREMENT ON  
SUBSTRATE MEMBER

FIG.12

MEASUREMENT ON  
SUBSTRATE MEMBER